


Library Prep Using the “With-Bead” Method

Introduction

This protocol is based on the method of Meyer and Kircher (2010) with modifications to accommodate the capturing of divergent species. The “with-beads” method is also adopted in this protocol to increase the complexity of the library (Fisher et al., 2011). Higher yield of the library was found when using the “with-beads” method than using the regular cleanup methods (Fig. 1).

***For capturing multiplexed samples, such as many individuals from a population, we usually choose 500bp shearing size, do indexing PCR (inline) before pooling them together for capturing (see details in the text).**

a)

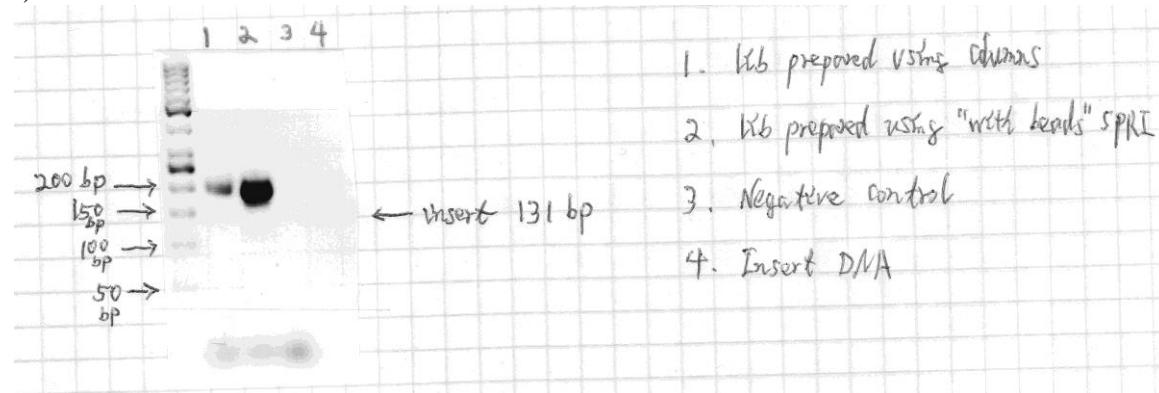

b)

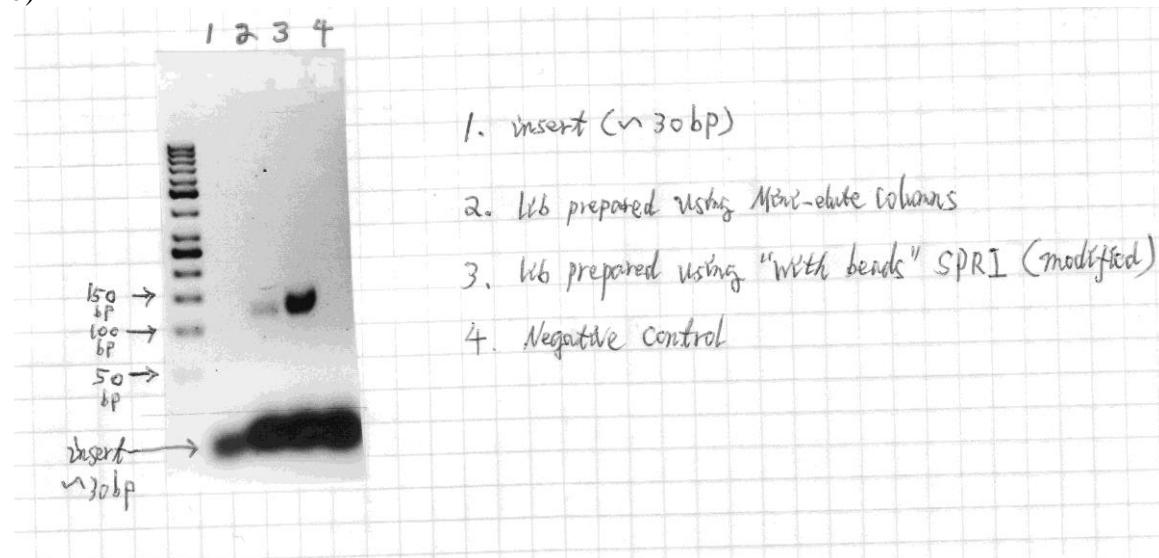


Fig.1. Comparison between “with-bead” library prep method and the common method using columns to cleanup the reaction after each step. a) library with insert size of 131 bp; b) library with insert size ~ 30 bp.

N.B.

It is very important to avoid potential cross-contamination. The following tips should be followed:

- *Clean your bench with bleach (84) every time after you did DNA extraction or fish dissection. Clean your pipettors, rack and bench space with bleach once a while.*
- *Aliquot all reagents into appropriate amount, so not to contaminate the whole tube of reagents.*
- *Make sure you have enough filtered tips, and never use tips without filter.*
- *Centrifuge the tube every time before you open a lid. Keep your finger off the inside of the lid. If you suspect that your gloves are contaminated, change it.*
- *Leave a space between tubes on rack, if you are not using multichannel pipettors.*
- *When pipetting, do it smoothly, don't pump it too fast. Keep the tip submerged just under the solution, so not push the liquid to overflow.*
- *When adding samples, set the tip against the wall of the tube.*
- *Move your tubes to an up row or switch the orientation of your tubes after adding samples to keep track which one has been added to.*
- *Keep focused; don't talk to others when they are working on sample prep.*

Library prep procedure

I. Shearing the genomic DNA

Skip the shearing step if using samples with highly degraded DNA, e.g., ancient DNA or DNA extracted from museum samples.

1. Start with 0.3 – 1 µg genomic DNA and shear it to ~ 250 bp range using the Covaris machine according to the instructions in “DNA Shearing on Covaris M220 with regular PCR tubes”.
** Use more DNA if available, e.g., 1 µg. Shear the DNA to ~ 500bp for multiplexing population level samples or if you want get longer flanking sequences.*
2. Centrifuge the tubes briefly. Check the size distribution of the sheared DNA on a mini agarose gel.
3. Dry down the sheared DNA using MagNA beads following the protocol “DNA Clean-Up Using MagNA Beads” (take **130** µL of sheared sample). Add **a positive (30 µL 10× 300bp DNA)** and **a negative (30 µL water)** control through all the rest of the steps.

II. Blunt-end repair

If working with ancient DNA or other samples with DNA fragment < 100 bp, skip the shearing step. Concentrate the DNA samples until dry using a speed vac.

Centrifuged the tubes briefly. Then add 20 µL of the master mix to each sample as in the protocol below. **Keep the tube stand for at least 1 hour.** After the blunt-end repair, skip step II-3. Instead, incubate the reaction at 75 °C for 20 min to deactivate the enzymes and followed by a ramp decreasing to 12 °C at the rate of 1 °C/s. Immediately proceed to the ligation step.

1. Prepare a master mix on an ice box for the number of samples needed as the follow. Add 20 µL of the master mix to each sample. Mix the sample well by pipetting 5-10 times smoothly.

Reagent	Volume (µL) per sample	× n	Final concentration in 20-µL reaction
Buffer Tango (10×)	2		1×
dNTPs (10 mM each)	0.2		100 µM each
ATP (100 mM)	0.2		1 mM
T4 polynucleotide kinase (10 U/µL)	1		0.5 U/µL
T4 DNA polymerase (5 U/µL)	0.4		0.1 U/µL
H ₂ O	16.2		
Total	20		

2. Incubate the samples in a thermal cycler for 15 min at 25 °C followed by 5 min at 12 °C. **Spin down the liquid by brief centrifugation.**
3. Clean up the reaction according to the MagNA beads protocol (add appropriate amount of PEG buffer to the sample, **no need to add new beads**). **Keep the dried beads.**

*Proceed immediately to the ligation step.

III. Adapter ligation

1. Prepare a master mix on an ice box for the number of samples needed (**inline adapters added later**).

Reagent	Volume (µL) per sample	× n	Final concentration in 40-µL reaction
T4 DNA ligase buffer (10×)	4		1×
PEG-4000 (50%)	4		5%
Inline Adapter mix IS1 (50 µM each)			1.25 µM each
Inline Adapter mix IS2 (50 µM each)			1.25 µM each
T4 DNA ligase (5 U/µL)	1		0.125 U/µL
H ₂ O	29		

Total	38
<i>If working with ancient DNA or other samples with DNA fragments < 100 bp, add 11 µL of water instead of 29 µL as in the protocol above, then add 20 µL of master mixture to each sample.</i>	

2. Add **38** µL of the master mix to each sample tube. Mix the samples well by pipetting 5-10 times smoothly.
 3. **Added inline adapter mix IS1 and IS2, 1 µL** of each to the sample tube according to sample sheet.
 4. Incubate for 30 min at 22 °C in a thermal cycler. Spin down the liquid by brief centrifugation.
 5. Cleanup the reaction using the MagNA bead method (add appropriate amount of buffer to the sample, **no need to add new beads**). **Keep the dried beads.**
- *Proceed immediately to the next step.**

IV. Fill-in

1. Prepare a master mix on an ice box for the number of samples needed.

Reagent	Volume (µL) per sample	× n	Final concentration in 40-µL reaction
Bsm buffer (10×)	4		1×
dNTPs (10 mM each)	1		250 µM each
Bsm polymerase, large fragment (8 U/µL)	1.5		0.3 U/µL
H ₂ O	33.5		
Total	40		

2. Add **40** µL of master mix to the samples. Mix the samples well by pipetting 5-10 times smoothly. Incubate the samples for 20 min at 37 °C. **Collect the liquid at the bottom of the tube by briefly centrifuging.**
 3. Cleanup the samples using the MagNA beads method. Add **35 µL** of TE buffer to each sample tube, **keep the beads within the tube**. Transfer the sample with the beads to a new tube labeled as “sample name + lib”.
- *The libraries now can be kept frozen at -20 °C for a short period of time.**

V. Pre-hybridization PCR “with-beads”

1. Prepare a master mix as the follow for the number of samples needed.

Reagent	Volume (μL) per sample	$\times n$	Final concentration in 25- μL reaction
KAPA HiFi taq Ready Mix (2 \times)	12.5		1 \times
Primer IS7 (10 μM)	0.75		0.3 μM
Primer IS8 (10 μM)	0.75		0.3 μM
Total	14		

2. Put the empty sample tubes on an iced box. Add **14 μL** of master mix to empty tubes, and then add **11 μL** of “lib” samples (take the **liquid mixed with beads** from the tube). Mix well and amplify the samples using the following thermal profile: 98 °C for 45 sec, **12 ~ 18** cycles of 98 °C for 15 sec, 60 °C for 30 sec and 72 °C for 45 sec, then followed by 72 °C for 1 min, and hold at 4 °C for 10 min. The number of PCR cycles can be adjusted according to the starting material used to construct the library.

**Keep the number of PCR cycles less than 18 cycles. Excessive amplification could increase the quantity of the PCR product but would also introduce more errors and bias.*

3. Cleanup the PCR product using the MagNA bead method [**add new beads and buffer**, because the high temperature (>90°C) in the PCR step may damage the coated layer of the previous beads]. Elute the DNA using **25 μL** of TE buffer and transfer the supernant to a new tube labeled as “**sample name + preH**”.
4. **Gel electrophoresis to check the amplified products, use 1 μL product.**
5. **Measure the concentration using Nanodrop3300.** The concentration of the samples should be around 20-30 ng/ μL . Store the preH product in -20 °C.

**Do the preH PCR just before the next gene capturing step to avoid degradation of library DNA. Pool the individual samples equimolarly if working with multiplexing population level samples. Do not pool more than 24 samples in each tube.*

Target enrichment – library preparation

*Don't do more than **32 samples** a time for lib prep and gene capture. Keep a list of index information for all samples. We have **24 pairs of inline index and 200 P7 index**. After capture, each tube should be amplified with different P7 indexed adapter. Here is an example of sample list:*

Tube	Sample	P5 inline index	P7 inline index	P7 adapter index
1	1	IS1_1	IS2_25	index_8nt_27
	2	IS1_2	IS2_26	
	3	IS1_3	IS2_27	
	4	IS1_4	IS2_28	
	5	IS1_5	IS2_29	
	6	IS1_6	IS2_30	
	7	IS1_7	IS2_31	
	8	IS1_8	IS2_32	
	9	IS1_9	IS2_33	
	10	IS1_10	IS2_34	
	11	IS1_11	IS2_35	
	12	IS1_12	IS2_36	
	13	IS1_13	IS2_37	
	14	IS1_14	IS2_38	
	15	IS1_15	IS2_39	
	16	IS1_16	IS2_40	
	17	IS1_17	IS2_41	
	18	IS1_18	IS2_42	
	19	IS1_19	IS2_43	
	20	IS1_20	IS2_44	
2	21	IS1_21	IS2_45	index_8nt_100
	22	IS1_22	IS2_46	
	23	IS1_23	IS2_47	
	24	IS1_24	IS2_48	
	25	IS1_1	IS2_26	
	26	IS1_2	IS2_27	
	27	IS1_3	IS2_28	
	28	IS1_4	IS2_29	
	29	IS1_5	IS2_30	
	30	IS1_6	IS2_31	
3	31	IS1_7	IS2_32	index_8nt_208
4	32	IS1_8	IS2_33	index_8nt_236
5	33	IS1_9	IS2_34	index_8nt_336
6	34	IS1_10	IS2_35	index_8nt_526
7	35	IS1_11	IS2_36	index_8nt_527
8	36	IS1_12	IS2_37	index_8nt_533
9	37	IS1_13	IS2_38	index_8nt_685
10	38	IS1_14	IS2_39	index_8nt_702

N.B.

- *This step is very important, wear gloves and a mask, and spin it down after each mixing, be very careful with potential cross-contamination.*
- *Premix the oligo hybridization buffer (10x) with H₂O according to 1 to 7 ratio; add 80 µL of the mixture into empty tubes. Then, add the adapters.*

Recipe for adapter mix

1. Assemble the following hybridization reactions in separate PCR tubes:

Hybridization mix for adapter P5 (50 µM, labeled as IS1_index):

Reagent	Volume (µL)	Final concentration in 100-µL reaction
IS1_adapter_P5.F (500 µM)	10	50 µM
IS3_adapter_P5+P7.R (500 µM)	10	50 µM
Oligo hybridization buffer (10×)	10	1×
H ₂ O	70	

Hybridization mix for adapter P7 (50 µM, labeled as IS2_index):

Reagent	Volume (µL)	Final concentration in 100-µL reaction
IS2_adapter_P7.F (500 µM)	10	50 µM
IS3_adapter_P5+P7.R (500 µM)	10	50 µM
Oligo hybridization buffer (10×)	10	1×
H ₂ O	70	

2. Mix and incubate the reactions in a thermal cycler for 10 sec at 95 °C, followed by a ramp from 95 °C to 12 °C at a rate of 0.1 °C/sec. [The original recipe (Meyer and Kircher, 2010) uses 200 µM for each adapter, we change it to 50 µM to save the cost].

3. Aliquot the mixture to different set of tubes (20 µL each), keep them at -20 °C.

Recipe for oligo hybridization buffer (10X)

Reagent	Volume (µL)	Final concentration in 10 ml
NaCl (5 M)	1 ml	500 mM
Tris-Cl, pH 8.0 (1 M)	100 µL	10 mM
EDTA, pH 8.0 (0.5 M)	20 µL	1 mM
H ₂ O	8.88 ml	

Sequences of adapters, and primers

Name	Sequences
IS1_adapter.P5	a*c*a*c*TCTTCCCTACACGACGCTCTCCg*a*t*c*
IS2_adapter.P7	g*t*g*a*CTGGAGTTCAGACGTGTGCTCTCCg*a*t*c*t
IS3_adapter.P5+P7	a*g*a*t*CGGAa*g*a*g*c
IS4_indPCR.P5	AATGATA CGGC GACC ACCGAG ATCTAC ACTCTTCCCTACACGACGCTCTT
IS5_reamp.P5	AATGATA CGGC GACC ACCGA
IS6_reamp.P7	CAAGCAGAAGACGGCATACGA
IS7_short_amp.P5	ACACTCTTCCCTACACGAC
IS8_short_amp.P7	GTGACTGGAGTT CAGACGTGT
IS4_n (P5)	AATGATA CGGC GACC ACCGAG ATCTACAC Cxxxxxxxxx AACTCTTCCCTACACGACGCTCTT
index_8nt_n (P7)	CAAGCAGAAGACGGCATACGAGATxxxxxxxxx GTGACTGGAGTT CAGACGTGT

Inline barcodes

Name	Sequences
IS1_Ind1	A*C*A*C*TCTTCCCTACACGACGCTCTCCGATCTtc*t*g*c*c
IS3_Ind1	ggcagaAGATCGGAA*G*A*G*C
...	
IS2_Ind25	G*T*G*A*CTGGAGTT CAGACGTGTGCTCTCCGATCTga*c*c*t*t
IS3_Ind25	aaggtaAGATCGGAA*G*A*G*C
...	

* indicates a PTO bond

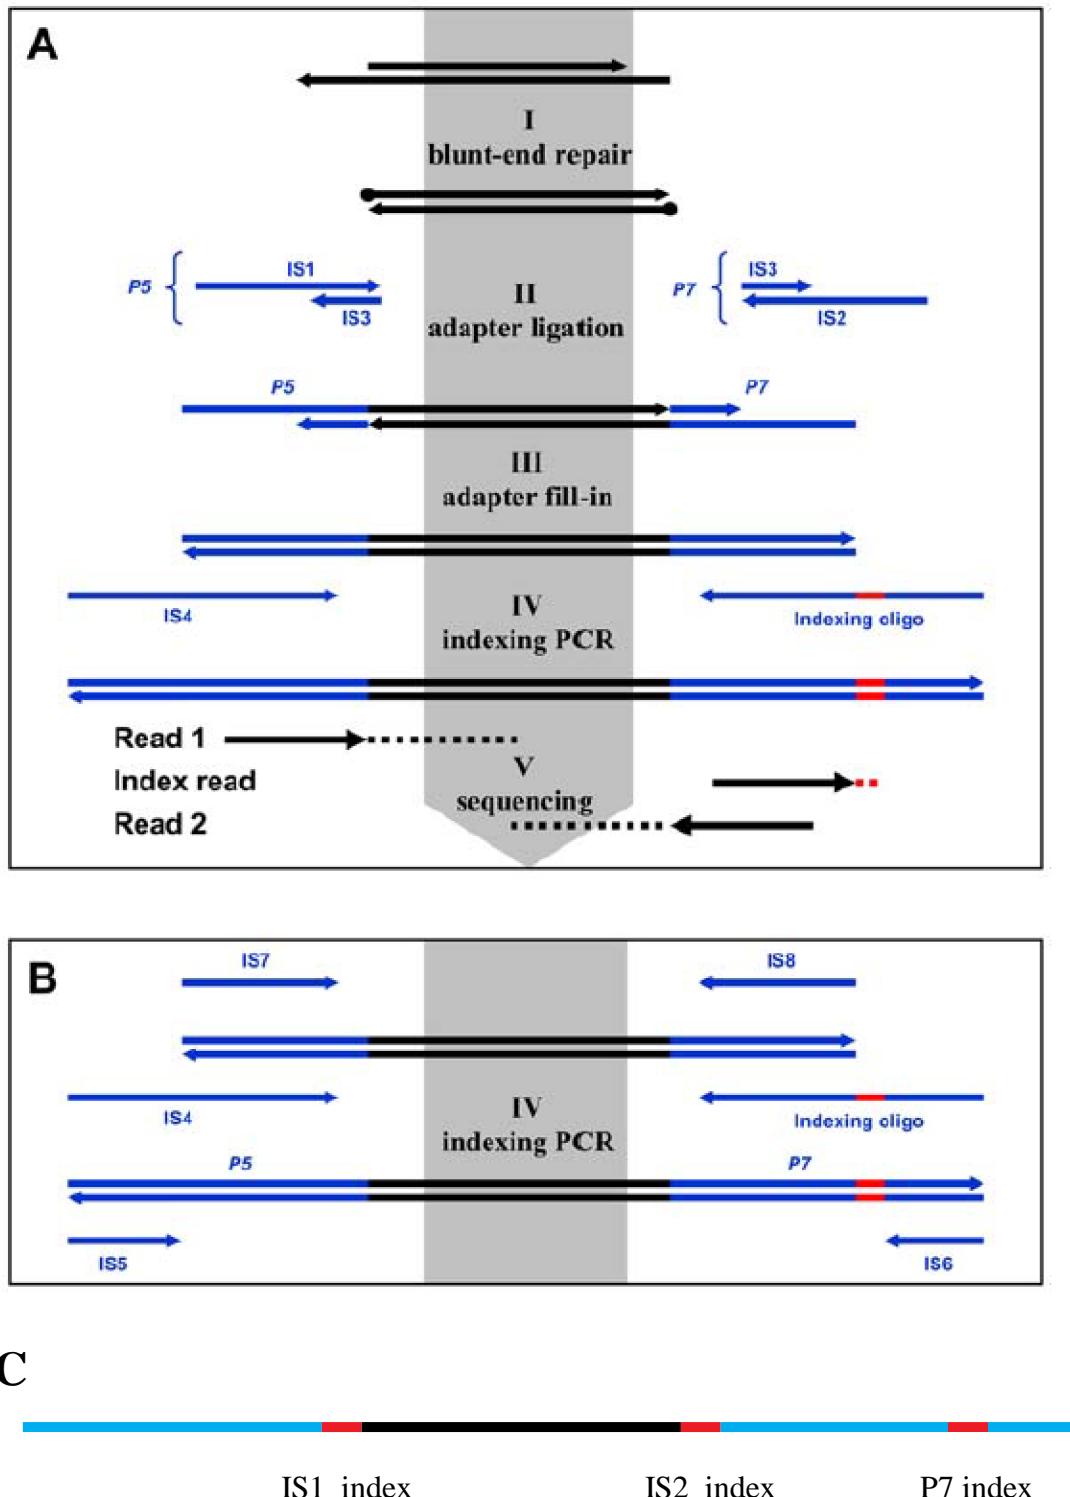


Fig.2. Schematic overview of the protocol and alternative amplification schemes (Meyer and Kircher, 2010). C shows the inline index (red).